

Instructions for Use: Instrument Protector Card

Brand Name of Product	Instrument Protector Card		
Generic Name of Product	Instrument Protector Card		
Product Code Number(s)	IPC001, IPC002, IPC003		
Intended Use	To protect delicate items		
Range of Applications for Product	Various sized items.		
Key Specifications of Product	<ul style="list-style-type: none">Made from solid bleached sulfate (SBS)– 265 g/m²<i>Paper:</i> Expandable base accommodates curved/larger instrumentsSingle-use		
	Instrument Protector Sizes:		
	Instrument Name	Instrument Size	Dimensions
	IPC001	Large	5.5- x 9.50 inches
	IPC002	Medium	3.5- x 6.75 inches
	IPC003	Small	1.75- x 8.25 inches

Shipping & Storage	
Shipping Conditions & Requirements	N/A
Storage Conditions	<ul style="list-style-type: none"> Store in dry conditions (20 – 60 rh%) at indoor room temperature 15- to 30 °C (59- to 86 °F). Store in original packaging or in an equivalent clean barrier to maintain cleanliness.
Packaging Contents	100 cards each box.
Shelf Life	N/A

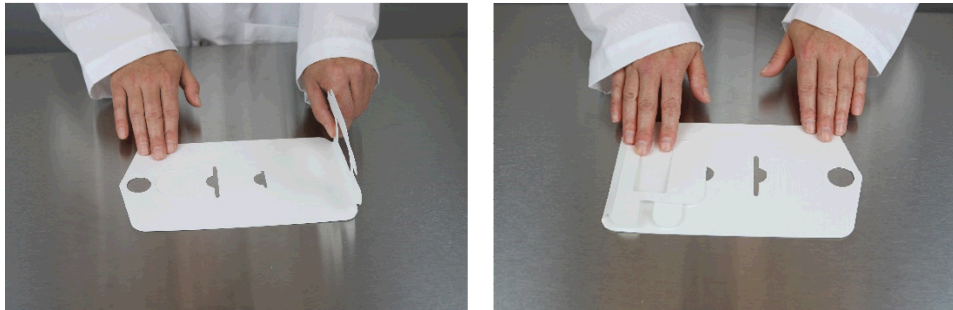
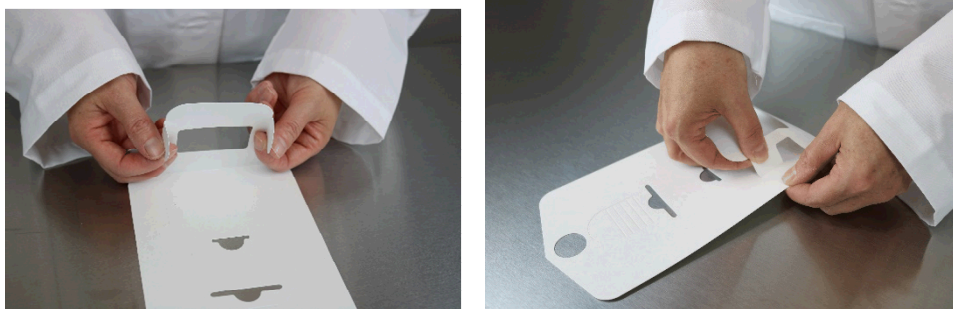
Instructions for Using Product	
Description of Use(s)	To protect items during sterilization, storage, and transportation. For use in sterile barrier systems.
Preparation for Use	N/A
Diagrams (drawings, pictures)	 <p style="text-align: center;">Figure 1</p>  <p style="text-align: center;">Figure 2</p>



Figure 3a



Figure 3b

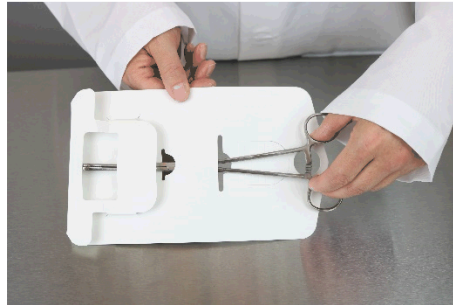


Figure 3c

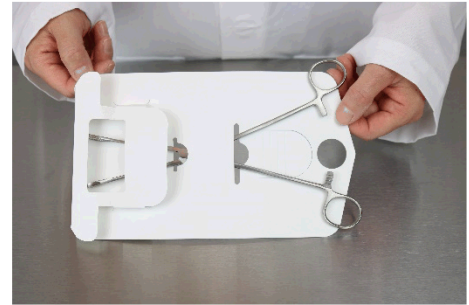


Figure 3d

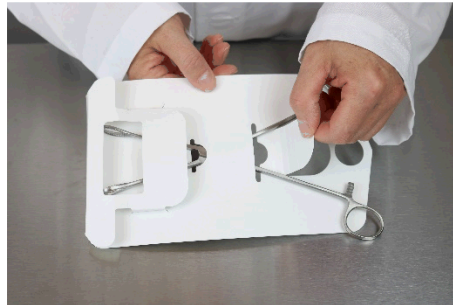


Figure 3e

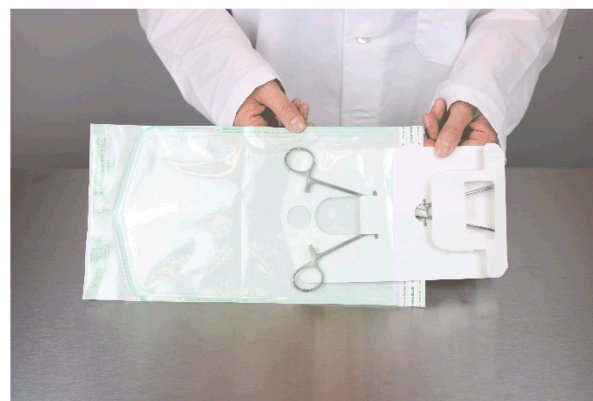
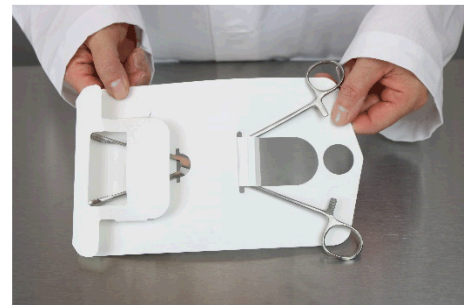


Figure 4

Steps for Use of Product

1. Fold bottom flap 180°. (**Fig 1**).
2. Fold the locking tabs and insert into the two-tab receiving slots at the bottom of the Instrument Protector. (**Fig 2**).
3. Place instrument into Instrument Protector.
 - a. Feed instrument through large “top hat” slot to the backside of card. (**Fig. 3a**).
 - b. Then feed instrument upward through the small “top hat” slot to the front of the card. (**Fig. 3b**).
 - c. Position instrument by working the distal end of the instrument into bottom fold-over pocket. (**Fig. 3c**).
 - d. Open instrument (if applicable) so that arms extend to outer most boundary of the large “top hat” slot. (**Fig. 3d**).

	<p>e. Fold tongue down over instrument arms and through the “top hat” slot (pull tight to secure instrument). (Fig. 3e).</p> <p>4. If using a peel pack, place Instrument Protector Card with finger hole oriented toward the chevron side. (Fig. 4).</p>
Interpretation of Test Results	N/A
Contraindications of Test Results	N/A
Documentation	N/A
Special Warnings and Cautions	Instrument Protector Cards are not a barrier to sterilant or a sterile barrier.
Disposal	<i>Single-use:</i> Dispose of in compliance with facility guidelines.

Reprocessing Instructions	
Point of Use	N/A
Preparation for Decontamination	N/A
Disassembly Instructions	N/A
Cleaning – Manual	N/A
Cleaning – Automated	N/A
Disinfection	N/A
Drying	N/A
Maintenance, Inspection, and Testing	N/A
Reassembly Instructions	N/A
Packaging	N/A
Sterilization	<ul style="list-style-type: none"> • <i>Compatible with steam sterilization:</i> <ul style="list-style-type: none"> ○ 132 °C (270 °F) for 4 minutes ○ 135 °C (275 °F) for 3 minutes • <i>Extended cycle:</i> 135 °C for 30 minutes • Material compatibility with EO sterilization
Storage	<ul style="list-style-type: none"> • Keep in dry conditions (20 – 60 rh%) and indoor room temperatures 15- to 30 °C (59- to 86 °F). • Keep in original packaging or in an equivalent clean barrier to maintain cleanliness.
Additional Information	N/A
Related Healthmark Products	Window Style Tip Protectors, Vented Instrument Guards, Duo-Vented Instrument Guards, Cylindrical Style, Instrument Guards.
Other Product Support Documents	ProSys™ Brochure, ProSys™ Price List
Reference Documents	N/A
Customer Service Contact	Healthmark Industries Company, Inc. 18600 Malyn Blvd. Fraser, MI 48026 1-586-774-7600 healthmark@hmark.com hmark.com