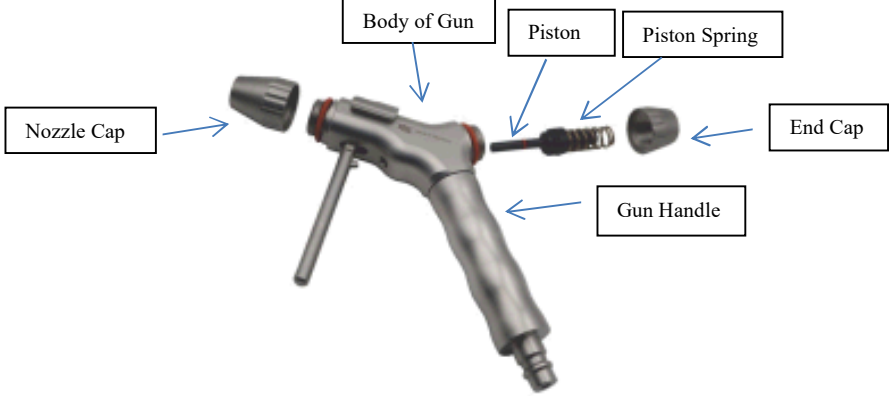


Instructions for Use: Stainless-Steel Spray Gun

Brand Name of Product	Stainless-Steel Spray Gun
Generic Name of Product	Spray Gun
Product Code Number(s)	64-20810-00
Purpose of Product	For cleaning an item with water or air.
Range of Applications for Product	N/A
Key Specifications of Product	<ul style="list-style-type: none"> Stainless steel construction: Variable flow control. Swap tips easily for different applications. Technical data: <ul style="list-style-type: none"> Medium: Oil-free compressed air/cold deionized water Max pressure: 0.5 MPa (5 bar or 72.5 psi).

Shipping & Storage	
Shipping Conditions & Requirements	N/A
Storage Conditions	N/A
Packaging Contents	N/A
Shelf Life	N/A

Instructions for Using Product	
Description of Use(s)	For rinsing items; particularly the internal channels.
Preparation for Use	The cleaning gun unit must be installed by a trained specialist in accordance with guidelines applicable depending on the intended use.
Diagrams (drawings, pictures)	 <p>The diagram shows an exploded view of the spray gun. Labels with arrows point to the following parts: Nozzle Cap (pointing to the cap on the left), Body of Gun (pointing to the main handle assembly), Piston (pointing to the small cylindrical part), Piston Spring (pointing to the spring behind the piston), End Cap (pointing to the cap on the right), and Gun Handle (pointing to the trigger handle).</p>
Steps for Use of Product	<ol style="list-style-type: none"> (Prior to operation), ensure any attachments are correctly seated on the safety conell by firmly pushing them onto the Spray Gun's rinse tip. <ol style="list-style-type: none"> ⚠ Caution: Do not point the spray gun at parts/orifices of the body. Compressed water/air jet may be harmful. Suitable safety measures/PPE (e.g., protective goggles, protective mask, etc.) must be taken to protect the user from splashes of contaminated water depending on the field of application. Set the maximum water or air pressure value using the small threaded nut located behind the trigger handle (<i>if required</i>). Control the flow by pulling the trigger up to the maximum set point fixed by the threaded nut.
Interpretation of Results	N/A
Contraindications of Test Results	N/A
Documentation	N/A
Special Warnings and Cautions	<ul style="list-style-type: none"> ⚠ Caution: Do not point the spray gun as parts/offices of the body because the compressed water or air jet may be harmful. Wear proper PPE according to facility and industry guidelines.

	<ul style="list-style-type: none"> ⚠ Caution: Oils containing white oil or paraffin oil will damage the O-rings. The enclosed silicone oil is not sterile. Any tubing used by the facility (other than that supplied by Healthmark) should be independently verified for safe and effective performance. In such a case, the facility assumes liability for the operation of the Spray Gun. Warranty: Components purchased only from Healthmark will be considered for warranty claims The Spray Gun is not a medical product and should not be used as part of medical treatments.
Disposal	N/A

Reprocessing Instructions	
Point of Use	N/A
Preparation for Decontamination	<ol style="list-style-type: none"> After the instrument parts are completely cleaned and dried, check the parts for possible defects. Perform sterilization in a single, transparent sterilization package.
Disassembly Instructions	N/A
Cleaning – Manual	N/A
Cleaning – Automated	<ol style="list-style-type: none"> <i>Pre-cleaning:</i> Cleaning agents for Spray Gun parts should be neutral detergent. Clean the parts in the cleaning solution with a soft brush and by fully immersing them into the liquid to remove all visible contamination. <i>Ultrasonic cleaning:</i> This is imperative! <ol style="list-style-type: none"> <i>Cleaning agents for instruments:</i> Depending on the level of contamination 1–3%. <i>Duration of ultrasonic cleaning:</i> 15 minutes. <i>Water temperature:</i> room temperature, but not exceeding 40 °C. The ultrasonic device must be suitable for the cleaning of medical instruments and should have a frequency of 35–40 kHz. The cleaning duration is to be extended when devices with a higher frequency are used. All instrument parts must be fully immersed in the cleaning solution and all hollow spaces must be filled. Ultrasonic baskets may not be overloaded as this could lead to acoustical shadows and the cleaning effect could not be guaranteed! <i>Rinsing:</i> Remove all chemical residues with water which is free from pathogenic germs. <i>Drying:</i> Dry all parts with nonlinting wipe and medical compressed air. Check the cleaning effect.
Disinfection	N/A
Drying	Dry all parts with nonlinting wipe and medical compressed air. Check cleaning and drying.
Maintenance, Inspection, and Testing	<p><u>Assembly of Spray Gun</u></p> <ol style="list-style-type: none"> Lubricate the front end of the piston and the small piston O-ring with pure silicone oil prior to the assembly. <ol style="list-style-type: none"> Use only minimal lubrication. Insertion of a dry piston will damage the piston seal. Insert the piston into the Spray Gun body. Position the piston spring onto the lubricated piston and screw the end cap to the gun body. Screw the nozzle cap to the front of the gun body, and screw the desired nozzle into the nozzle cap. Screw the gun handle into the gun body as far as it will go. If it is difficult to insert it into or remove it from stainless-steel coupling, lubricate the plug nipple of the handle DN7.2 with pure silicone oil. <p><u>Disassembling the cleaning gun:</u></p> <ol style="list-style-type: none"> Disassemble the endcap from the body of the gun by turning it counterclockwise. Remove the piston spring. Pull back trigger and pull the piston out backwards.

	<ol style="list-style-type: none"> Loosen nozzles from nozzle cap by turning them counterclockwise. Disassemble the nozzle cap from the body of the gun by turning it counterclockwise. Disassemble the handle from the body of the gun by turning it counterclockwise. Disassemble the shower nozzle sieve from the shower nozzle body by turning it counterclockwise. <p><u>Reassembly of the cleaning gun to the gun coupling:</u></p> <ol style="list-style-type: none"> Introduce the gun handle with coupling plug DN7.2 straight into the gun coupling and press it in until it audibly engages into position. Open the pressure supply line. Check the whole system for leakage. <p><u>Dismounting the cleaning gun from the gun coupling:</u></p> <p>If you want to dismount the cleaning gun from the coupling again for reprocessing, you must interrupt the pressure supply.</p> <ol style="list-style-type: none"> Relieve the pressure in the hose by activating the gun trigger. After pressure is relieved, press the gun handle into the coupling and simultaneously pull the sliding ring and top of coupling down toward the hose. Then, pull the gun out of the coupling. Put the sterile coupling protection cap over the gun coupling. The hose must be stored in such a way that it does not come into contact with liquids and cannot be contaminated. Clean and sterilize the coupling protection cap the same way as the cleaning gun parts. <p>Maintenance</p> <ul style="list-style-type: none"> It is recommended to decalcify the Spray Gun approximately every 4 weeks. <ol style="list-style-type: none"> Disassemble the Spray Gun and place its inner parts in an approved decalcifying agent. This is beneficial for the service life and reliability of the Spray Gun. If it is difficult to remove the cg piston from the gun body or insert it into the gun body, then you must replace the small O-ring for the cg piston. Replacement parts and instructions for repair are available from Healthmark.
Reassembly Instructions	N/A
Packaging	N/A
Sterilization	N/A
Storage	N/A
Additional Information	⚠ Caution: Oils containing white oil or paraffin oil will damage the O-rings.

Related Healthmark Products	N/A
Other Product Support Documents	N/A
Reference Documents	ProSys™ Brochure, ProSys™ Price List
Customer Service Contact	Healthmark Industries Company, Inc. 18600 Malyn Fraser, MI 48026 1-586-774-7600 healthmark@hmark.com hmark.com