healthmark
INDUSTRIES CO.
health care products
800-521-6224
www.hmark.com

Instructions for Use: ScopeDryCheck™

Brand Name of Product	ScopeDry Check™
Generic Name of Product	ScopeDryCheck™
Product Code Number(s)	SDC-001
Intended Use	To test lumens/channels for detectable levels of residual moisture.
Range of Applications for Product	For any lumened/channeled items.
Key Specifications of Product	• MEASURING RANGE: The ScopeDryCheck™ can detect down to 50nL or 0.05µL of residual moisture. • ScopeDryCheck™ Card - 3.5W x 2H Inches • Response time 2 to 5 seconds

Shipping & Storage	
Shipping Conditions & Requirements	Avoid exposure to moisture.
Storage Conditions	Store in a cool dry place at 60-80°F with RH of 30-60%. Avoid exposure to moisture.
Packaging Contents	N/A
Shelf Life	2 years from the date of manufacturer.

Instructions for Using Product	
Description of Use (s)	To test lumens/channels for detectable levels of residual moisture.
Preparation for Use	N/A
Diagrams (drawings, pictures)	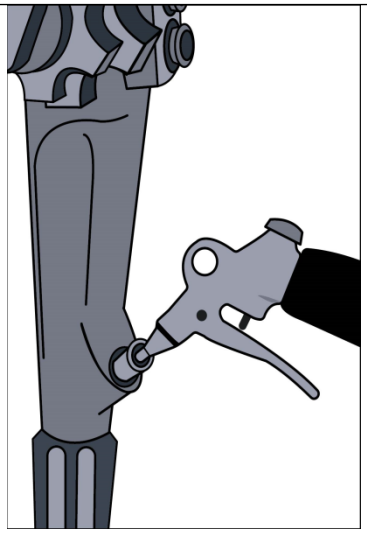 **Figure 1** 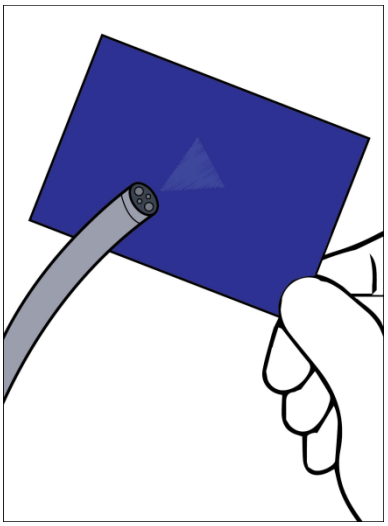 **Figure 2A**

	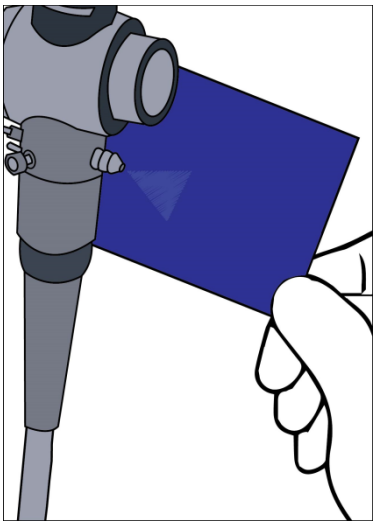 **Figure 2B** 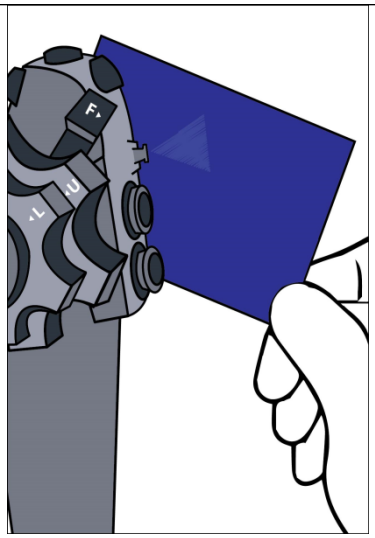 **Figure 2C** 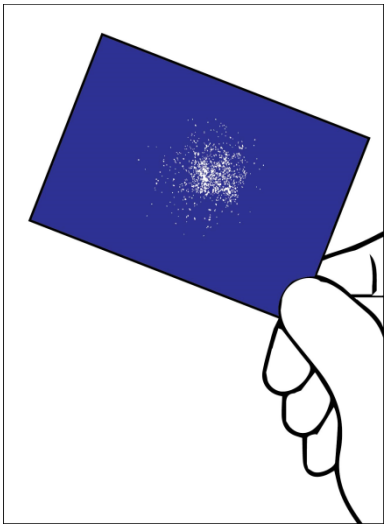 **Figure 3**
Steps for Use of Product	1. With dry gloved hands, after drying any lumen/channeled items according to the manufacturer's IFU, with the same air source used to dry the scope, flush air through the biopsy port. 2. On the flipside of the card, with a gloved hand hold the ScopeDryCheck™ in one of the corners with the blue side up ready to test if the lumen/channel is dry, while blowing air, aim the scope 1 cm away from the card in the following sequence: A. Distal end- Flush air through the biopsy port. **Fig. 1, 2A** B. Suction connector- Flush air through the suction valve port. **Fig. 2B** C. Auxiliary water inlet- Flush air through the suction valve port. **Fig. 2C** 3. If any white dots are visible at any time during this test procedure, resume drying of the item, then retest with a new card. **Fig. 3** 4. Repeat test until no white dots are visible.
Interpretation of Test Results	If white dots are visible on the card, the item is not dry. Repeat drying steps and retest with another area of the card to check for residual moisture.
Contraindications of Test Results	N/A
Documentation	N/A
Special Warnings and Cautions	N/A
Disposal	Single-use, dispose of according to healthcare facility policy.

Reprocessing Instructions	
Point of Use	N/A
Preparation for Decontamination	N/A
Disassembly Instructions	N/A

Cleaning – Manual	N/A
Cleaning – Automated	N/A
Disinfection	N/A
Drying	N/A
Maintenance, Inspection, and Testing	N/A
Reassembly Instructions	N/A
Packaging	N/A
Sterilization	N/A
Storage	N/A
Additional Information	N/A
Related Healthmark Products	N/A
Other Product Support Documents	ProFormance™ Brochure, ProFormance™ Price List
Reference Documents	N/A
Customer Service Contact	Healthmark Industries Company, Inc. 18600 Malyn Blvd. Fraser, MI 48026 1-586-774-7600 healthmark@hmark.com hmark.com